

HAMILTON-T1

Technical specification for SW 2.2.x

Ventilation modes

Mode form	Mode name	Mode	Adult/Ped	Neonatal
Volume-targeted	APVcmv / (S)CMV+	Breaths are volume targeted and mandatory.	✓	✓
modes, adaptive pressure controlled	APVsimv / SIMV+	Volume-targeted mandatory breaths can be alternated with pressure-supported spontaneous breaths.	✓	✓
Pressure-controlled modes	PCV+	All breaths, whether triggered by the patient or the ventilator, are pressure-controlled and mandatory.	✓	✓
	PSIMV+	Mandatory breaths are pressure controlled. Mandatory breaths can be alternated with pressure-supported spontaneous breaths.	✓	✓
	DuoPAP	Mandatory breaths are pressure controlled. Spontaneous breaths can be triggered at both pressure levels.	0	0
	APRV	Spontaneous breaths can be continuously triggered. The pressure release between the levels contributes to ventilation.	0	0
	SPONT	Every breath is spontaneous, with or without pressure-supported spontaneous breaths.	✓	✓
Intelligent ventilation	ASV	Operator sets %MinVol, PEEP, and Oxygen. Frequency, tidal volume, pressure, and I:E ratio are based on physiological input from the patient.	✓	--
Noninvasive modes	NIV	Every breath is spontaneous.	0	0
	NIV-ST	Every breath is spontaneous as long as the patient is breathing above the set rate. A backup rate can be set for mandatory breaths.	0	0
	nCPAP	Demand flow Nasal Continuous Positive Airway Pressure.	--	0
	nCPAP-PC	Breaths are pressure controlled and mandatory.	--	0
High flow oxygen therapy	HiFlowO2	High flow oxygen therapy. No supported breaths.	0	0

Standard: ✓ Option: 0 Not applicable: --

Standard configuration and options (in alphabetical order)

Functions	Adult/Ped	Neonatal
Capnography, mainstream (volumetric) and sidestream	o	o
Communication ports: COM1 port, USB port, Nurse call	o	o
Communication protocols: for details see Connectivity brochure	o	o
Dynamic Lung	✓	--
Event log (up to 1000 events with data and time stamp)	✓	✓
Handles for various options (jet, ambulance, or bed rail mount)	o	o
IntelliTrig (leak compensation)	✓	✓
Languages (English, US-English, Chinese, Croatian, Czech, Danish, Dutch, Finnish, French, German, Greek, Hungarian, Indonesian, Italian, Japanese, Korean, Norwegian, Polish, Portuguese, Romanian, Russian, Serbian, Slovak, Spanish, Swedish, Turkish)	✓	✓
Manual breath/prolonged inspiration	✓	✓
NBC filter (only for HAMILTON-T1 Military)	o	o
Nebulization, pneumatic	✓	--
Night Vision Goggles (NVG) option	o	o
O2 enrichment	✓	✓
Oxygen adjustable from 21% to 100%	✓	✓
Patient group	✓	o
Print screen	✓	✓
Screen lock	✓	✓
Second battery (hot-swappable)	o	o
Speak valve compatibility	o	--
SpO2 monitoring	o	o
Standby with timer	✓	✓
Suctioning tool	✓	--
Trends/Loops	o	o
Flow trigger	✓	✓
Vent Status (Visual representation of ventilator dependence)	✓	✓

Standard: ✓ Option: o Not available: --

Technical performance

Description	Specification
Automatic expiratory base flow	Adult/Ped: Fixed at 3 l/min Neonatal: Fixed at 4 l/min
Inspiratory pressure	0 to 60 cmH ₂ O
Maximum inspiratory flow	260 l/min (120 l/min with 100% O ₂)
Minimum expiratory time	20% of cycle time; 0.2 to 0.8 seconds
Means of inspiratory triggering	Flow trigger control
Oxygen mixer accuracy	± (volume fraction of 2.5% + 2.5% of actual reading)
Preoperational checks	Tightness test, Flow Sensor/O ₂ sensor/CO ₂ sensor calibration
Tidal volume	Adult/Ped: 20 to 2000 ml Neonatal: 2 to 300 ml
Brightness setting for display	The range is 10% to 100% brightness. By default, Day is set to 80%; Night is set to 40%.
Brightness with NVG option	The range is 1 to 10. The default is 5.

Standards and approvals

Classification	Class IIb, continuously operating according to EC directive 93/42/EEC
Certification	IEC 60601-1:2005/A1:2012, IEC 60601-1-2:2014, ANSI/AAMI ES60601-1:2005/(R)2012, ISO 80601-2-12:2011, CAN/CSA-C22.2 No. 60601-1:14, EN ISO 5356-1:2015, ISO 80601-2-55:2011
Declaration	The HAMILTON-T1 was developed in accordance with pertinent international standards and FDA guidelines. The ventilator is manufactured within an EN ISO 13485 and EN ISO 9001, Council Directive 93/42/EEC, Annex II, Article 3 certified quality management system. The ventilator meets the Essential Requirements of Council Directive 93/42/EEC, Annex I.
Electromagnetic compatibility	According IEC 60601-2:2014
Air transport compatibility	EN1789:2007+A2:2014, EN 13718-1:2014, EN 794-1:1997 +A2:2009, RTCA/DO-160G, MIL-STD-461F, MIL-STD-810G, Chg. 1, Meth 500.6, Proc. II Operation/Air Carriage, mod.
Safety Class	Class II, Type B applied part (ventilator breathing system, VBS), type BF applied part CO ₂ sensor including CO ₂ module connector; SpO ₂ sensor including adapter, continuous operation according to IEC 60601-1

Pneumatic performance

High-pressure O ₂	Pressure:	2.8 to 6 bar / 41 to 87 psi
	Connector:	DISS (CGA 1240) or NIST
Low-pressure O ₂	Pressure:	Maximum 6 bar / 87 psi
	Connector:	Quick-coupling system, compatible with Colder Products Company (CPC) PMC series
Air supply	Integrated turbine	
Inspiratory outlet (To patient port)	Connector:	ISO ID15/OD22 conical
Expiratory outlet (From patient port)	Connector (on expiratory valve)	ISO ID15/OD22 conical

Electrical specifications

Input power	100 to 240 VAC \pm 10%, 50/60 Hz 12 to 28 VDC (total range 10.2 to 30.3 VDC)
Power consumption	50 VA typical, 150 VA maximum
Battery	Electrical specifications: 10.8 V DC, 6.7 Ah, 72 Wh, 50 W typical, 150 W maximum Type: Lithium-ion, supplied by Hamilton Medical only Normal operating time: Typically 4 hours with one battery, 8 hours with two batteries One battery, display brightness = 80%: 4 h One battery, display brightness = 20%: 4.5 h Two batteries, display brightness = 80%: 8 h Two batteries, display brightness = 20%: 9.25 h

Graphical patient data

Graphic type/tab name	Options
Waveforms	Pressure, Volume, Flow, PCO ₂ ¹ , FCO ₂ ¹ , Plethysmogram ²
Intelligent panels	Dynamic Lung ³ , Vent Status, ASV Graph ⁴
Trends	1-, 6-, 12-, 24-, or 72-h ⁵ trend data for a selected parameter or combination of parameters
Loops	Pressure/Volume, Pressure/Flow, Volume/Flow, Volume/PCO ₂ ¹ , Volume/FCO ₂ ¹

Alarms⁶

Priority	Alarm
High priority	Apnea time (s), ExpMinVol high/low (l/min), Oxygen high/low (%), Pressure high/low (cmH ₂ O), Flow sensor calibration needed, Exhalation obstructed, Disconnection, Oxygen supply failed
Medium priority	fTotal high/low (b/min), PetCO ₂ high/low (mmHg), Pressure limitation (cmH ₂ O), Vt high/low (ml), SpO ₂ high/low, High PEEP, Loss of PEEP, Pulse high/low
Low priority	High SpO ₂ , Loss of external power

¹ CO₂ option required.

² SpO₂ option required.

³ Only for adult/pediatric patients.

⁴ Only in ASV mode.

⁵ 72-hour trend not available in all markets.

⁶ For a complete list of alarms, see your ventilator Operator's Manual .

Control settings and ranges⁷

Parameter (units)	Range Adult/Ped	Range Neonatal
Apnea backup	On, Off	On, Off
ETS (%)	5 to 80	5 to 80
Flow (l/min)	2 to 80 ⁸	2 to 12
Flow trigger (l/min)	1 to 20	0.1 to 5
Height (cm)	30 to 250	--
Height (in)	12 to 98	--
I:E	1:9 to 4:1	1:9 to 4:1
%MinVol (%)	25 to 350	--
Oxygen (%)	21 to 100	21 to 100
PEEP (cmH ₂ O)	0 to 35	3 to 25
Pasvlimit (cmH ₂ O)	5 to 60	--
Pcontrol (cmH ₂ O)	5 to 60	3 to 45
Phigh APRV (cmH ₂ O)	0 to 60	0 to 45
Phigh DuoPAP (cmH ₂ O)	0 to 60	3 to 45
Pinsp (cmH ₂ O)	3 to 60	3 to 45
Plow APRV (cmH ₂ O)	0 to 35	0 to 25
Pramp (ms)	0 to 2000	0 to 600
Psupport (cmH ₂ O)	0 to 60	0 to 45
Rate (b/min)	1 to 80	1 to 80
Sex	Male, Female	--
Sigh	On, Off	--
SpO ₂ monitoring	On, Off	On, Off
SpeakValve	On, Off	--
TI (s)	0.1 to 12	0.1 to 12
TI max (s)	1 to 3	0.25 to 3
Thigh APRV (s)	0.1 to 40	0.1 to 40
Thigh DuoPAP (s)	0.1 to 40	0.1 to 40
Tlow APRV (s)	0.2 to 40	0.2 to 40
Vt (ml)	20 to 2000	2 to 300
VtWeight (ml/kg)	--	5 to 12
Weight (kg)	--	0.2 to 30

⁷ Parameter settings and ranges can vary depending on the selected mode.


⁸ Flow limited to 60 l/min in some markets.

Monitoring parameters

Parameter (units)	Description		
Pressure	AutoPEEP (cmH ₂ O)	Unintended positive end-expiratory pressure	
	PEEP/CPAP (cmH ₂ O)	PEEP (positive end-expiratory pressure) and CPAP (continuous positive airway pressure)	
	P _{insp} (cmH ₂ O)	Inspiratory pressure	
	P _{mean} (cmH ₂ O)	Mean airway pressure	
	P _{peak} (cmH ₂ O)	Peak airway pressure	
	P _{plateau} (cmH ₂ O)	Plateau or end-inspiratory pressure	
Flow	Control Flow (l/min)	The set flow of gas to the patient when using HiFlowO ₂ .	
	Flow (l/min)	In nCPAP mode, the average flow, updated every second. In nCPAP-PC mode, the average flow during expiration, updated every breath.	
	Insp Flow (peak) (l/min)	Peak inspiratory flow, spontaneous or mandatory	
	Exp Flow (peak) (l/min)	Peak expiratory flow	
Volume	ExpMinVol or MinVol NIV (l/min)	Expiratory minute volume	
	MVSpont or MVSpont NIV (l/min)	Spontaneous expiratory minute volume	
	VTE or VTE NIV (ml)	Expiratory tidal volume	
	VTI (ml)	Inspiratory tidal volume	
	VLeak (%)	Leakage percent or total minute volume leakage	
	MVLeak (l/min)	Leakage percent or total minute volume leakage	
CO ₂	FetCO ₂ (%)	Fractional end-tidal CO ₂ concentration	
	PetCO ₂ (mmHg)	End-tidal CO ₂ pressure	
	slopeCO ₂ (%CO ₂ /l)	Slope of the alveolar plateau in the PetCO ₂ curve, indicating the volume/flow status of the lungs	
	V _{alv} (l/min)	Alveolar minute ventilation	
	V _{talv} (ml)	Alveolar tidal ventilation	
	V _{CO2} (ml/min)	CO ₂ elimination	
	VDaw (ml)	Airway dead space	
	VDaw/VTE (%)	Airway dead space fraction at the airway opening	
	VeCO ₂ (ml)	Exhaled CO ₂ volume	
	ViCO ₂ (ml)	Inspired CO ₂ volume	
	SpO ₂	SpO ₂ (%)	Oxygen saturation
		Pulse (1/min)	Pulse
SpO ₂ /FiO ₂ (%)		The SpO ₂ /FiO ₂ ratio (%) is an approximation of the PaO ₂ /FiO ₂ ratio, which, in contrast to PaO ₂ /FiO ₂ , can be calculated noninvasively and continuously.	
PI (%)		Perfusion index	
PVI (%)		Pleth variability index	
SpCO (%)		Carboxyhaemoglobin saturation	

Parameter (units)		Description
SpO2	SpMet (%)	Methaemoglobin saturation
	SpHb (g/dl or mmol/l)	Total haemoglobin
	SpOC (ml/dl)	Oxygen content
Oxygen	Oxygen (%)	Oxygen concentration of the delivered gas
	Oxygen consumption (l/min)	The current oxygen consumption rate
Time	I:E	Inspiratory:expiratory ratio
	fControl (b/min)	Mandatory breath frequency
	fSpont (b/min)	Spontaneous breathing frequency
	fTotal (b/min)	Total breathing frequency
	TI (s)	Inspiratory time
	TE (s)	Expiratory time
Lung mechanics	Cstat (ml/cmH2O)	Static compliance
	P0.1 (cmH2O)	Airway occlusion pressure
	PTP (cmH2O*s)	Pressure time product
	RCexp (s)	Expiratory time constant
	Rinsp (cmH2O / (l/s))	Inspiratory flow resistance
	RSB (1 / (l*min))	Rapid shallow breathing index

Physical characteristics

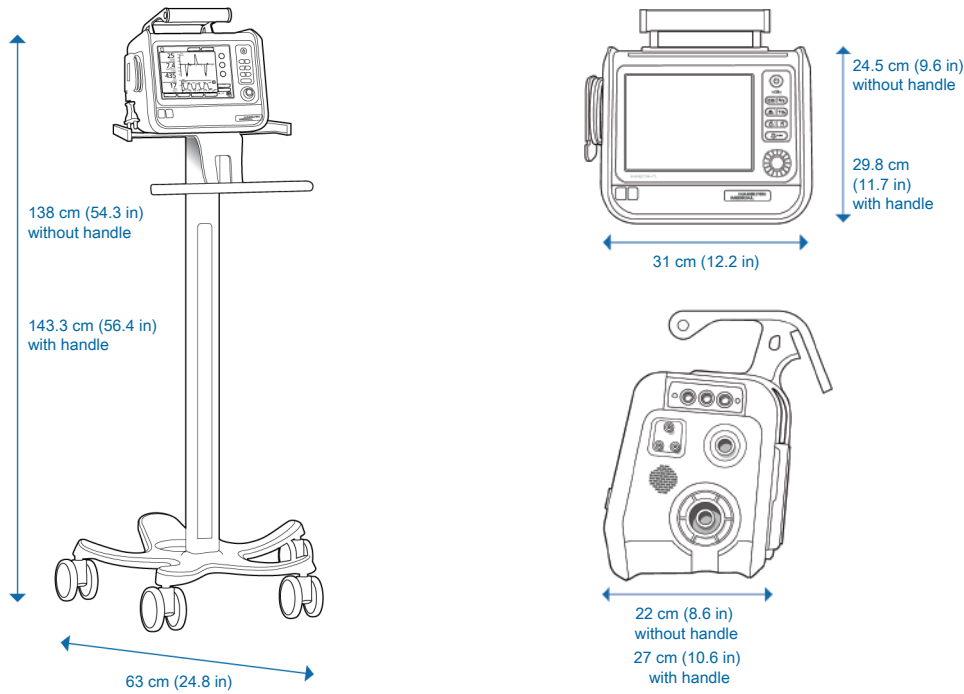

Weight	6.5 kg (14.3 lb) 18.5 kg (40.8 lb) with trolley The trolley can accommodate a maximum safe working load of 44 kg (97 lb)
Dimensions	See graphic above
Monitor	Type: TFT color Size: 640 x 480 pixels, 8.4 in (214 mm) diagonal
Trolley accessories	HAMILTON-H900 mounting system, optional O2 bottle holding system, optional tubing support arm